

Joint Preservation

# **Fixation**In a Flip



## **Fixation**

# In a Flip


#### **As Much Fixation As Needed**

The XCEL RC Bioabsorbable Anchor was designed for rotator cuff repairs. The 3.5mm anchor is loaded with two strands of #2 Force Fiber through separate suture eyelets to maximize suture management. The XCEL RC anchor is designed to be inserted into a small 3.5mm pilot hole, preserving much of the native bone. The surgeon gets tactile feedback during deployment when the anchor "flips" in sub-cortical bone and disengages from the inserter.




#### Features & Benefits:

- Anchor inserts at 3.5mm
- Separate suture eyelets




STEP 1:

• Create 3.5mm Pilot Hole




STEP 2:

• Insert Anchor to Horizontal Laser Mark



Pull back on Handle to Deploy Anchor



Repair Soft Tissue with Suture



## Above the Rest

#### **Easy Suture Management**

The XCEL RC Anchor's innovative "T-Handle" design allows the sutures to slide free from the inserter as it is pulled back during anchor deployment.

#### Features & Benefits:

- Tactile feedback upon deployment
- Anchor is rigidly attached to inserter until deployment
- Laser mark for insertion depth & eyelet orientation



Drill Guide PN. 3910-004-039



Suture slides through handle to disengage.

Force Fiber™ #2



Obturator PN. 3910-004-038




Awi PN. 3910-004-042



Drill PN. 3910-004-037

## **Suture Strength Comparisons**

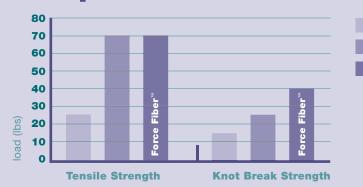

Developed in conjunction with:

Medicine Lodge, Inc.



Joint Replacements
Trauma, Extremities & Deformities
Craniomaxillofacial
Spine
Biologics
Surgical Products
Neuro & ENT
Interventional Pain
Navigation
Endoscopy
Communications
Imaging
Patient Handling Equipment
EMS Equipment

325 Corporate Drive Mahwah, NJ 07430 **t: 201 831 5000** 

www.stryker.com

A surgeon should always rely on his or her own professional clinical judgment when deciding to use which products and/or techniques on individual patients. Stryker is not dispensing medical advice and recommends that surgeons be trained in orthopaedic surgeries before performing any surgeries.

The information presented is intended to demonstrate the breadth of Stryker product offerings. Always refer to the package insert, product label and/or user instructions before using any Stryker product. Products may not be available in all markets. Product availability is subject to the regulatory or medical practices that govern individual markets. Please contact your Stryker representative if you have questions about the availability of Stryker products in your area.

Stryker Corporation or its divisions or other corporate affiliated entities own, use or have applied for the following trademarks or service marks: XCEL, Stryker.

All other trademarks are trademarks of their respective owners or holders.

Literature Number: 1000-900-600 Rev.A

MS/GS 05/08

Copyright © 2008 Stryker Printed in USA